

REPLACEMENT SHEET

6/14

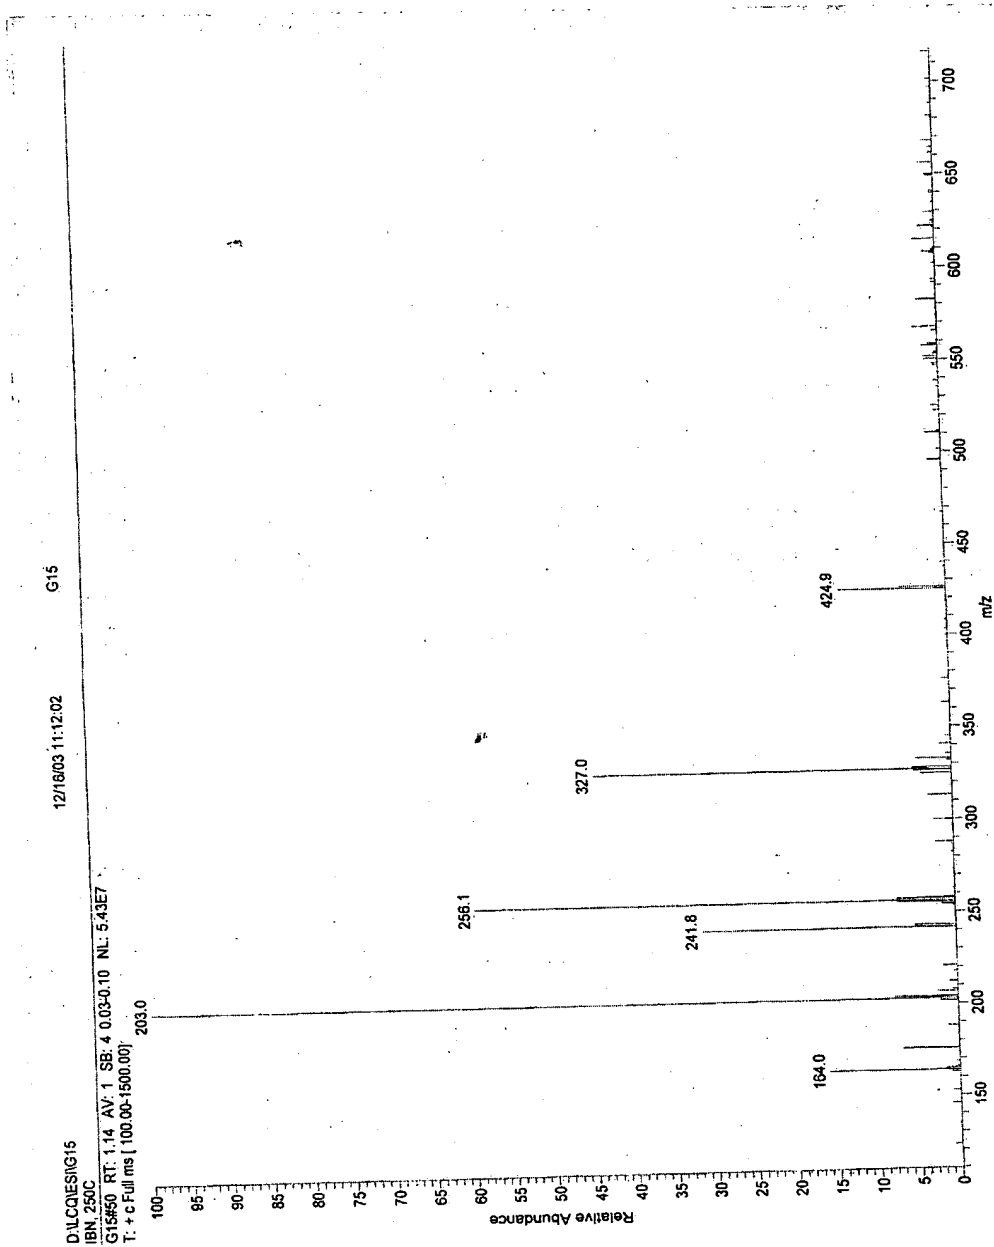


FIGURE 7A

BEST AVAILABLE COPY



7/14

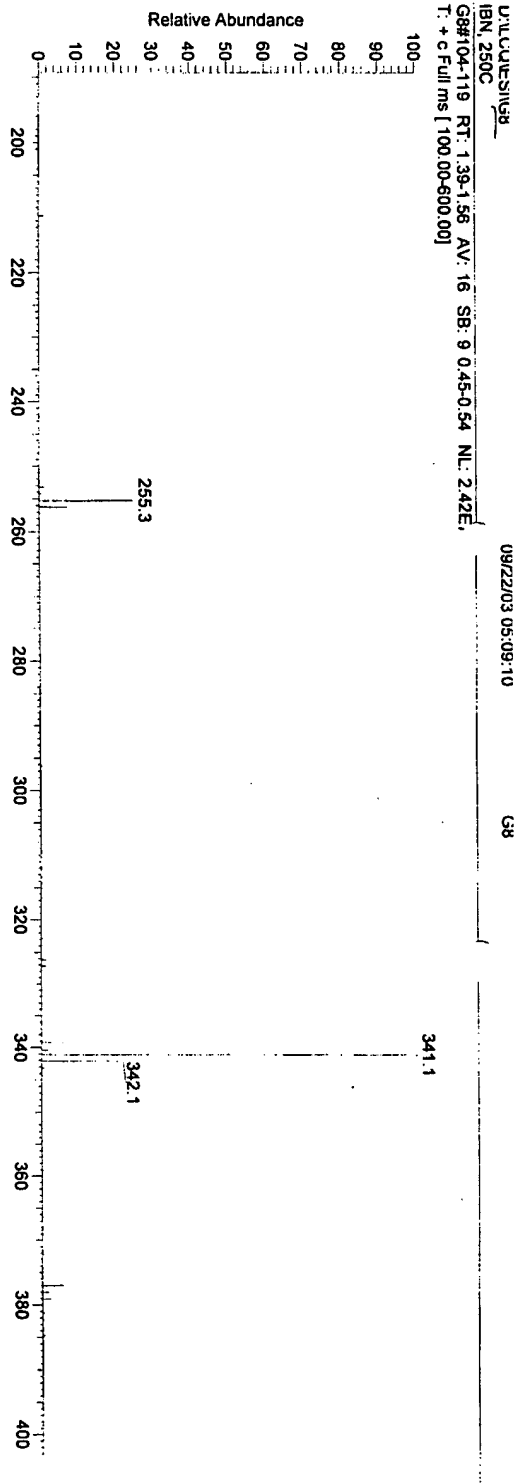


FIGURE 7B

10/14

IBN DR GAO ZHIQIANG 1H DPX300
GS (WITH WATER SUPPRESSION)

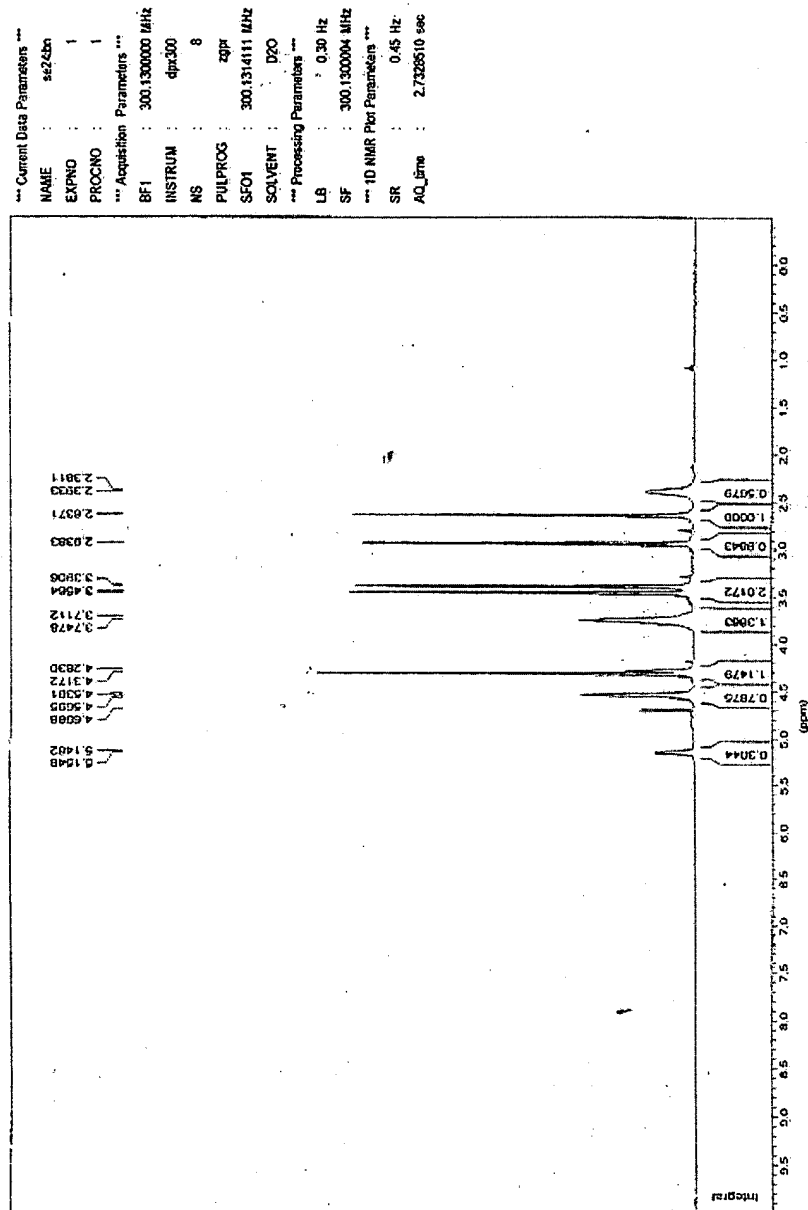


FIGURE 9A

BEST AVAILABLE COPY

11/14

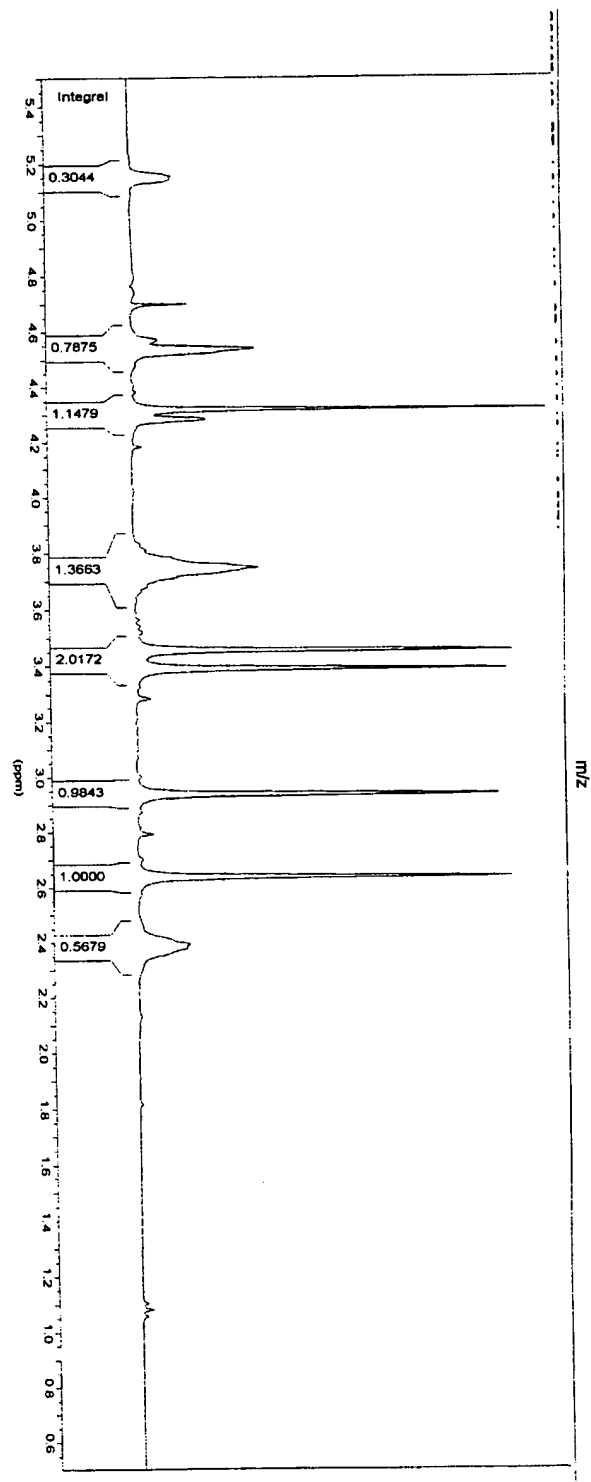


FIGURE 9B

BEST AVAILABLE COPY